

1. VRAE 4-gas meter



2. PhotoVac 20/20 PID




3. TSI DustTrak II





- 1. Solar Panel
- 2. DustTrak™ sample tubing with in-line condenser
- 3. DustTrak™ sample inlet with PM-10 impactor
- 4. Station enclosure
- 5. DustTrak™ Aerosol Monitor
- 6. PhotoVac™ 20/20 PID
- 9. PhotoVac™ 20/20 PID sample inlet
- 10. PhotoVac™ 20/20 PID sample inlet tubing
- 9. Data communications device



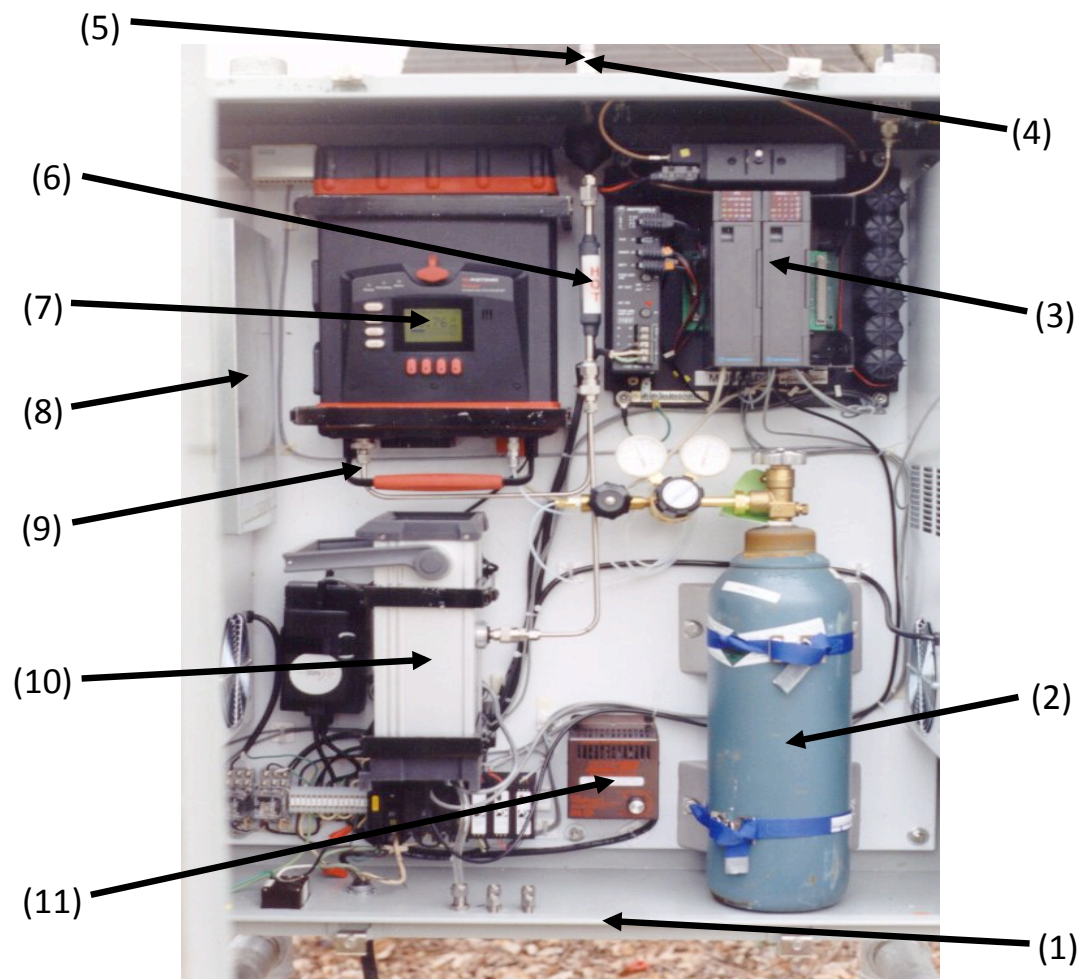

1. Station enclosure
2. GC carrier gas
3. Data communications device
4. GC sample inlet
5. DataRAM sample inlet with PM-10 impactor
6. DataRAM sample tubing with in-line heater
7. PhotoVac Voyager gas chromatograph (GC)
8. Heat exchanger
9. GC sample inlet tubing
10. MIE DataRAM portable real-time aerosol monitor
11. Heater element

